

### **Quick Facts**





# 4.0 mm Locking Screws Compatible with 3.5 mm plates, including TPLO plates

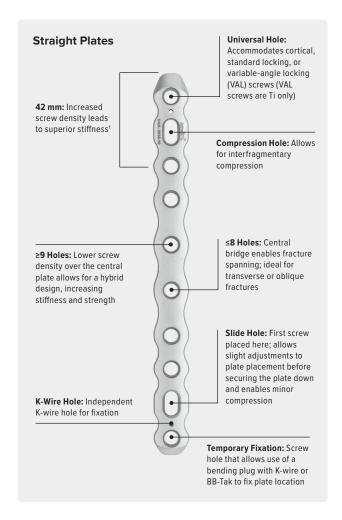

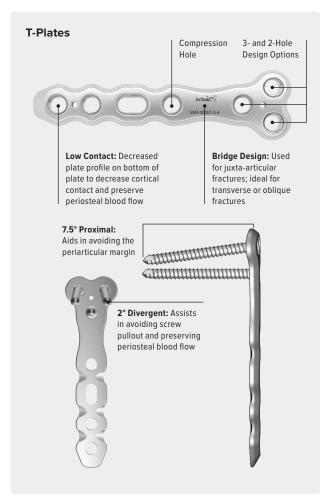

#### Reference


 Stoffel K, Dieter U, Stachowiak G, Gächter A, Kuster MS. Biomechanical testing of the LCP—how can stability in locked internal fixators be controlled? *Injury*. 2003;34 Suppl 2:B11-B19. doi:10.1016/j.injury.2003.09.021

### arthrexvetsystems.com

© 2025-05 Arthrex, Inc. All rights reserved. vBR1-004344-en-US\_D



### **Quick Facts**

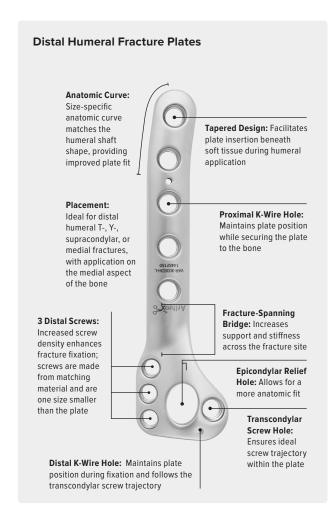





# QuickFix Cannulated Screws > Hexalobe drive > Titanium alloy > Partially threaded > Cannulated design > Fits through the transcondylar screw hole of the distal humeral plate; does not lock into the plate







### **Quick Facts**

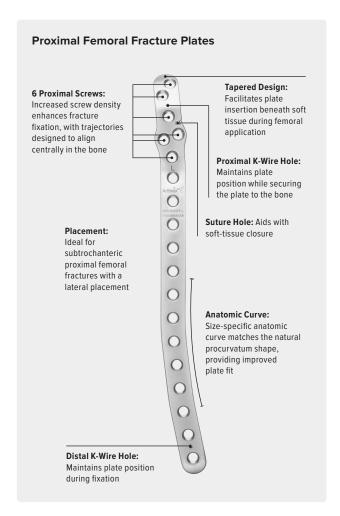


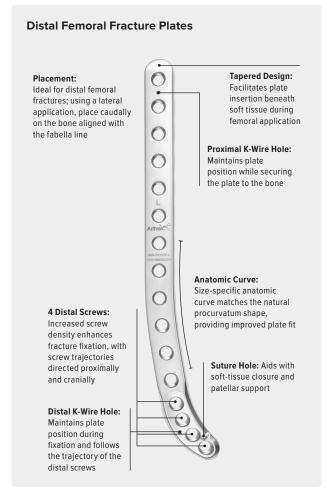


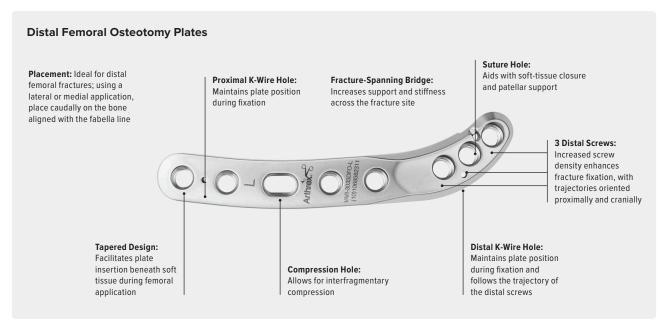

### **Quick Facts**

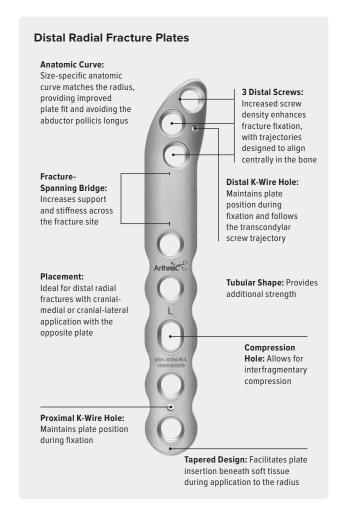

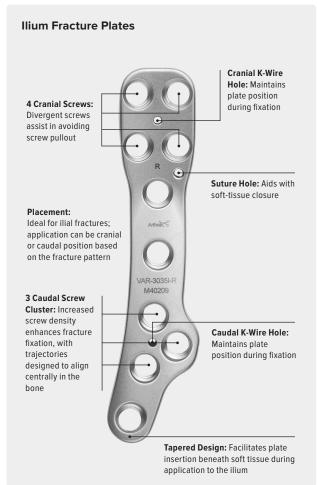

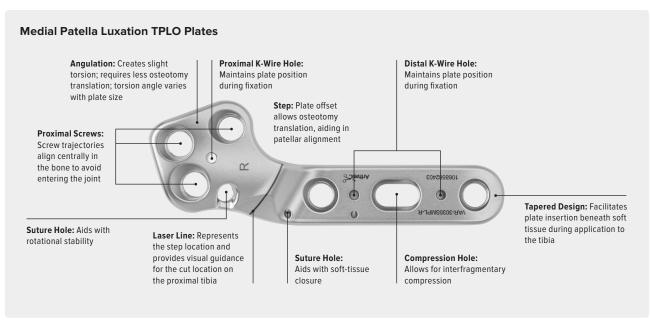

## OrthoLine™ Cuttable Plates

### **Quick Facts**

